


Smith+Nephew

AETOS[◇]
Shoulder System

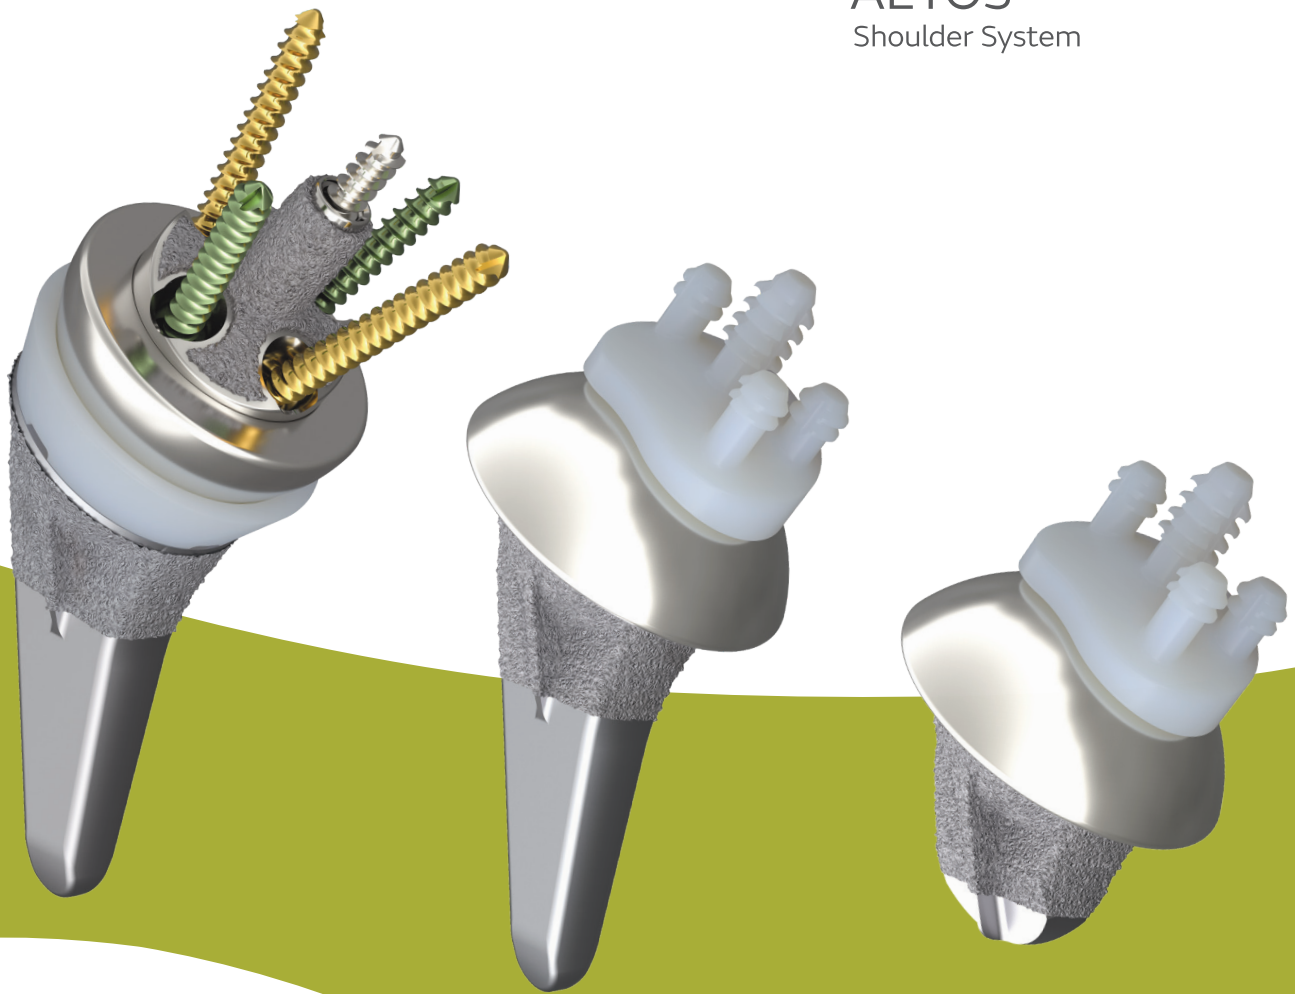

Elegant design.
Elevated experience.

AETOS[◇] Shoulder System

Move with mastery




AETOS Shoulder System

Designed to simplify the OR with a compact system.⁵ Perform a complete TSA or RSA with just 2 trays.




Anatomic Glenoid


4-peg oval shape designed to provide stability and resist rocking horse.^{1,2}

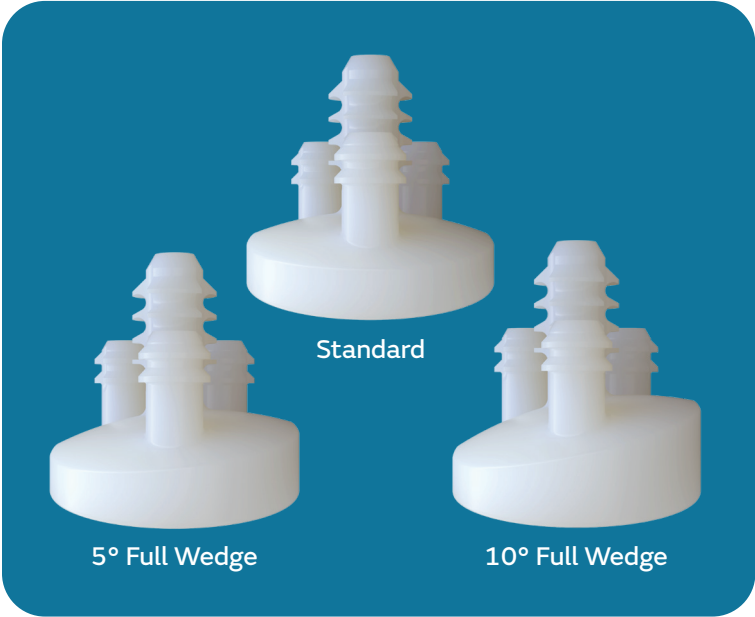

AETOS[◇] Meta Stem TSA

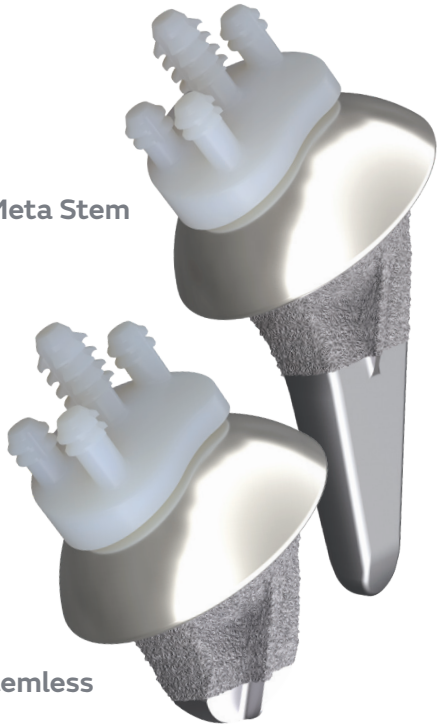


AETOS Stemless TSA

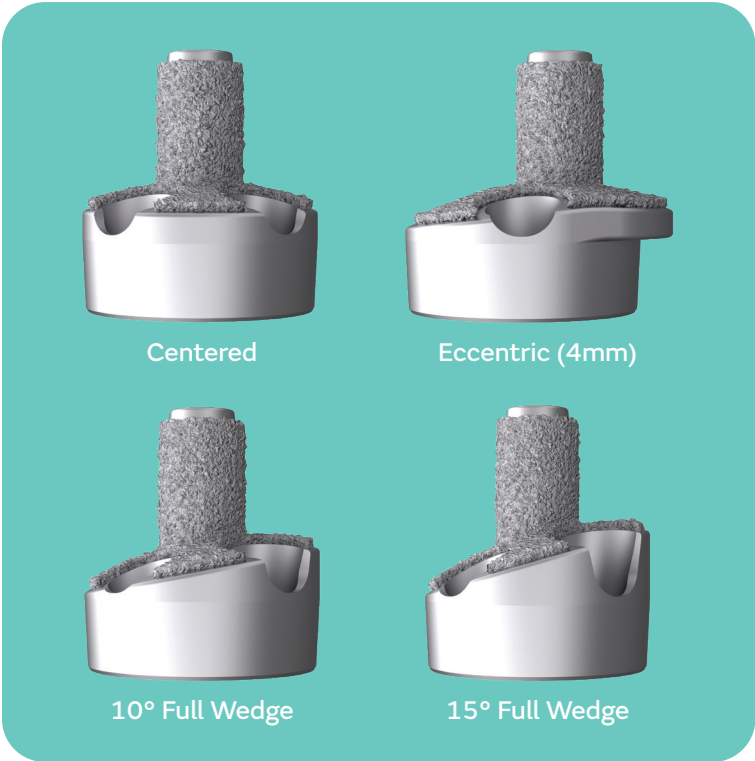

Baseplate

- The circular base plate design allows for implantation flexibility.
- Multiple wedge options are designed to help minimize reaming in glenoid defects.

AETOS Meta Stem RSA

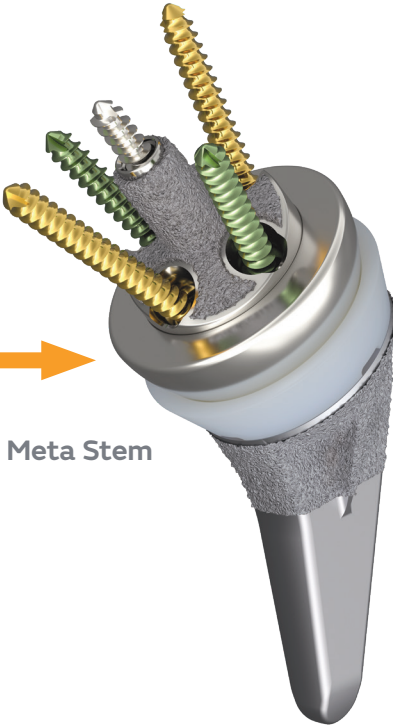

TITAN Modular Shoulder System

Integrated solutions for unique patient anatomy and fractures

- Intraoperative building platform and pathway for revision
- Modular system allows for independent selection of distal stems and proximal bodies that best match the patient's anatomy and bone quality
- Diaphyseal fit for fixation in variable bone



Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets. Please contact your Smith+Nephew representative or distributor if you have questions about the availability of Smith+Nephew products in your area. For detailed product information, including indications for use, contraindications, precautions and warnings, please consult the product's applicable Instructions for Use (IFU) prior to use.

Smith & Nephew, Inc.
1450 Brooks Road
Memphis, Tennessee 38116
USA

www.smith-nephew.com

®Trademark of Smith+Nephew
All Trademarks acknowledged
©2025 Smith & Nephew, Inc.
37284 V2 08/25

References

1. Smith+Nephew 2023. AETOS Glenoid Interdigitation Feature. Internal Report. ER-04-0990-0018.
2. Integra 2022. Aetos Anatomic Glenoid Loosening Report. Internal Report. ER-04-0990-0013 REV AA.
3. Smith+Nephew 2023. AETOS Inlay Design Features. Internal Report. ER-04-0990-0017.
4. Smith+Nephew 2023. AETOS Anatomic Humeral Head Design. Internal Report. ER-04-0990-0019.
5. Smith+Nephew 2023. AETOS Instruments & Trays. Internal Report. ER-04-0990-0020.