
T.I.M.E. clinical decision support tool PRESSURE INJURIES (treatment)



ΡΙ

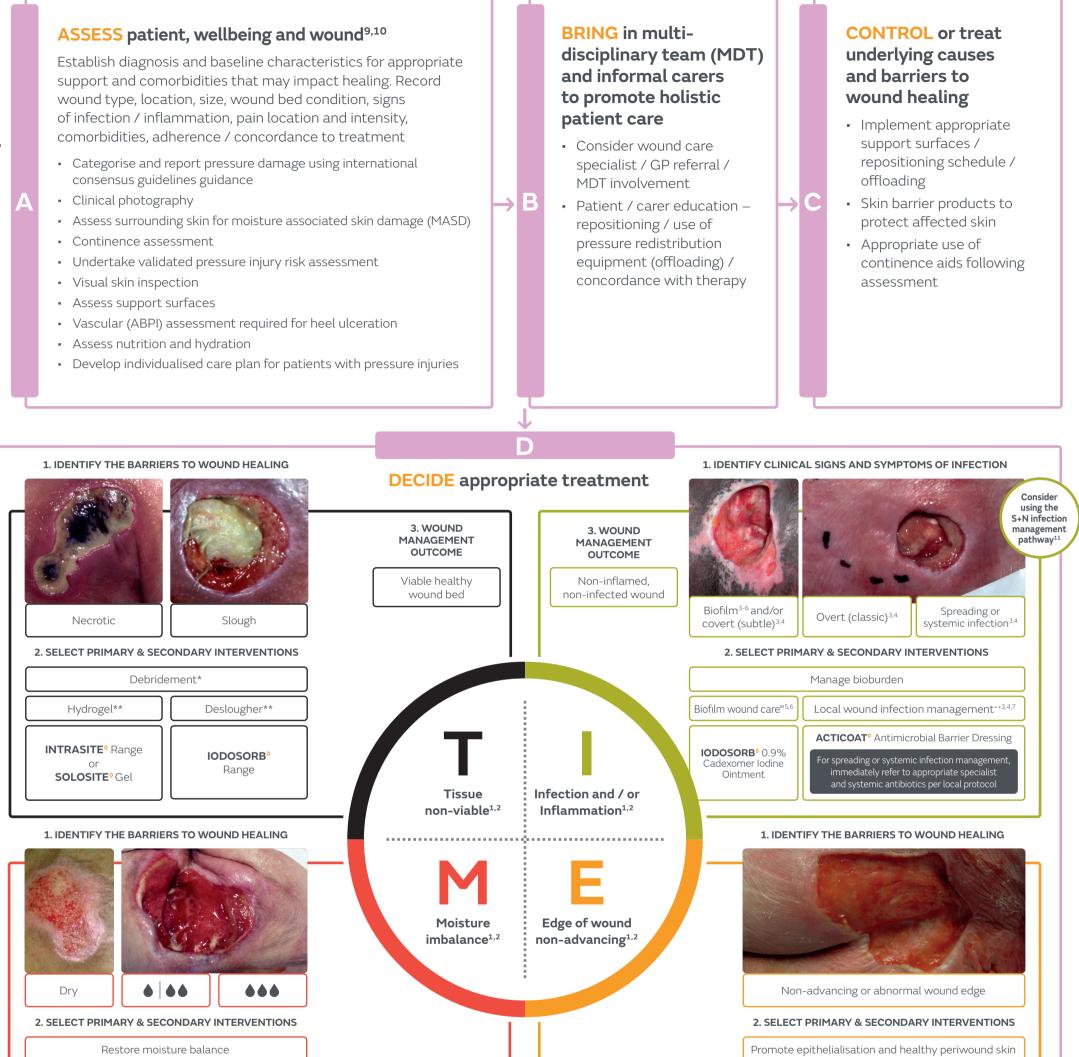

*Always ensure adequate blood supply before debriding necrotic tissue. **Use appropriate secondary dressing as per your local protocol. ***Consider whether wound edge debridement is also required.

EVALUATE and reassess the treatment and wound management outcomes

Evaluate: Record wound progression within given timelines.

Flag if no change, go back to A, B, C and change treatment where indicated. Repeat pressure injury risk assessment as per your protocol.

RECOMMENDATION: Non-wound care specialists need to be trained on T.I.M.E. Wound Bed Preparation and how to conduct comprehensive wound assessment. Developed with the support of Glenn Smith⁸ and Moore et al. 2019⁹

INTRASITE Range includes INTRASITE Gel and INTRASITE CONFORMABLE. ACTICOAT Range includes ACTICOAT and ACTICOAT FLEX. IODOSORB range includes ointment, powder and dressing †NPWT: Negative Pressure Wound Therapy. ‡Level of exudate for wounds suitable for NPWT. §SECURA Range includes SECURA No Sting Barrier Film. PROSHIELD Range includes PROSHIELD Plus and PROSHIELD Plus and Spray. ∞Biofilm wound care: Debridement, cleanse and use anti-biofilm agent. ++ Debride and cleanse and use effective topical antimicrobial as per local protocol.

Reference: 1. Schultz GS, et al. Wound Rep Reg (2003);11:1–28. **2.** Leaper DJ, et al. Int Wound J 2012; 9 (Suppl. 2):1–19. **3.** International Wound Infection Institute (IWII) Wound infection in clinical practice. Wounds International (2016). **4.** Weir D, Schultz G. Assessment and Management of Wound-Related Infections. In Doughty D & McNichol L (Eds.). Wound, Ostomy and Continence Nurses Society Core Curriculum: Wound Management (p. 156–180). 2016. Philadelphia: Wolters-Kluwer. **5.** Wolcott RD, et al. J Wound Care 2010;19(2):45–53. **6.** Schultz G, et al. Wound Repair Regen 2017;25(5):744–757. **7.** Ayello EA, et al. Wounds Int 2012;1–24. **8.** Smith G, et al. Journal of Wound Care 2010;19(9):396–402. **9.** Moore Z, et al. Journal of Wound Care, 2019;28(3):154–161. **10.** European Pressure Ulcer Advisory Panel, National Pressure Injury Advisory Panel and Pan Pacific Pressure Injury Alliance. Prevention and Treatment of Pressure Ulcers/Injuries: Clinical Practice Guideline. Emily Haesler (Ed.) EPUAP/NPIAP/PPIA: 2019. **11.** Dowsett C, et al. Wounds Int. 2020;11(3):20–27.

The products used in the T.I.M.E. clinical decision support tool may vary in different markets. Not all products referred to may be approved for use or available in all markets. Please consult your local Smith+Nephew representative for further details on products available in your market. Intended for healthcare professionals outside of the US only.

Smith+Nephew does not provide medical advice. The information presented is not, and is not intended to serve as, medical advice. For detailed device information, including indications for use, contraindications, precautions and warnings, please consult the product's Instructions for Use (IFU) prior to use. It is the responsibility of healthcare professionals to determine and utilise the appropriate products and techniques according to their own clinical judgment for each of their patients.

Smith+Nephew Pty Ltd, Australia, T +61 2 9857 3999, F +61 2 9857 3900 | Smith+ Nephew Ltd, New Zealand, T +64 9 820 2840, F +64 9 820 2841 Vrademark of Smith+Nephew. All Trademarks acknowledged. ©March 2022 Smith+Nephew. 29664-anz