

+ A low allergy dressing retention sheet for fixation of dressings and tubing¹

PRIMAFIX Hypoallergic Non-Woven Retention Tape: A conformable retention tape that ensures fixation without restricting patient movement*^{2,3}



Smith+Nephew

PRIMAFIX[◇]

Hypoallergenic Non-Woven
Retention Tape

www.smith-nephew.com

*As demonstrated in vitro

PRIMAFIX[◇] Hypoallergenic Non-Woven Retention Tape is a non-woven adhesive tape for fixation of primary dressings as well as catheter and drainage tubing.

Features and benefits

Patient friendly

PRIMAFIX Tape is a low allergy non-woven retention tape.¹

Conformable

PRIMAFIX Tape is conformable* ensuring reliable fixation, allowing joints to be dressed without constraining movement.^{2,3}

Permeable

PRIMAFIX Tape is permeable to moisture vapour to help prevent moisture build-up underneath the dressing.³

Easy of use

PRIMAFIX Tape can be cut for easy application.²

Radio transparent

PRIMAFIX Tape is radio transparent, meaning the dressing will not appear on x-ray images taken of the patient.⁴

*As demonstrated *in vitro*.


Indications

PRIMAFIX Hypoallergenic Non-Woven Retention Tape use is indicated for:

- Retention of post-operative wound dressings
- Retaining gauze and absorbent pads
- Secure catheter tubing and drainig tubes

PRIMAFIX Hypoallergenic Non-Woven Retention Tape

S+N Code	Size	Carton
66800151	5cm x 10m	1 roll
66800152	10cm x 10m	1 roll
66800153	15cm x 10m	1 roll
66800154	20cm x 10m	1 roll
66600151	5cm x 10m	1 roll
66600152	10cm x 10m	1 roll
66600153	15cm x 10m	1 roll
66600154	20cm x 10m	1 roll

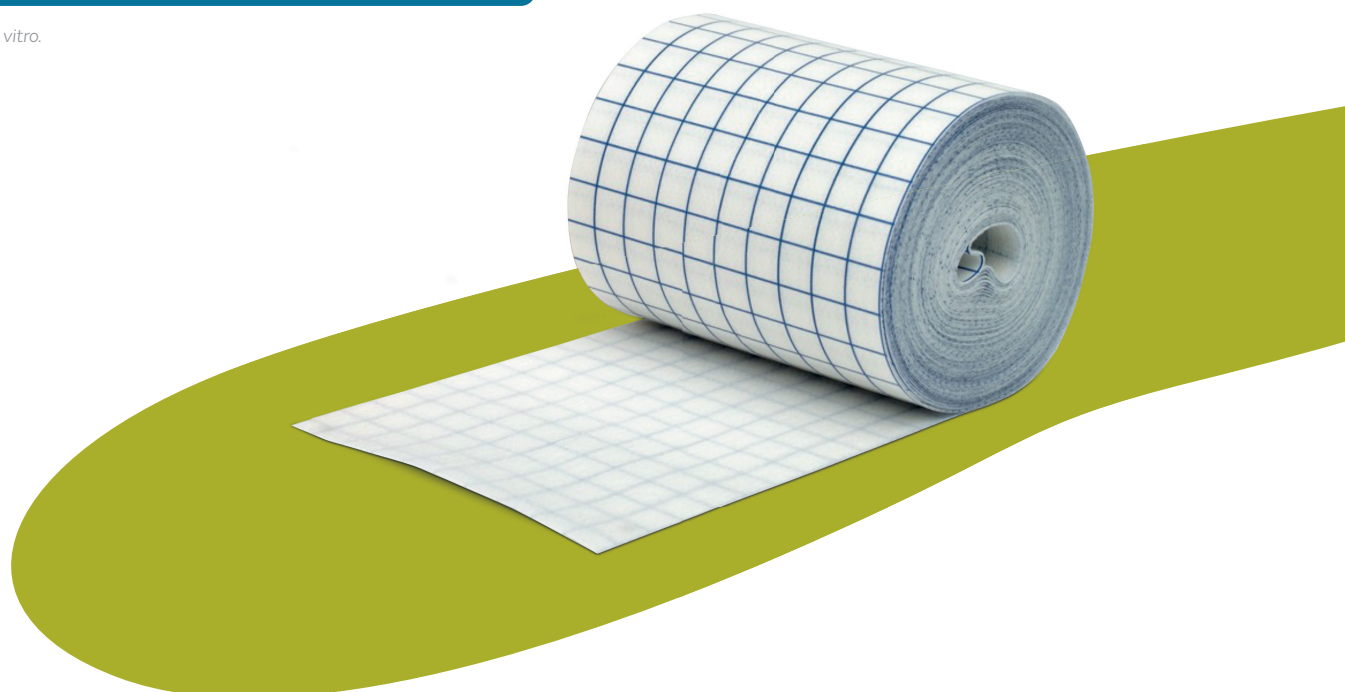

Advanced Wound Management
Smith & Nephew Medical Ltd
Croxley Park Building 5, Lakeside
Hatters Lane, Watford,
Hertfordshire WD18 8YE - UK
T +44 (0) 1923 477100
F +44 (0) 1923 477101

www.smith-nephew.com

[◇]Trademark of Smith+Nephew
All Trademarks acknowledged
©April 2022 Smith+Nephew
AWM-AWD-32695 | GMC1459

For detailed product information, including indications for use, contraindications, precautions and warnings, please consult the product's applicable Instructions for Use (IFU) prior to use.

References

1. Smith+Nephew 2018. Product Safety Statement. Internal statement. PSS304. 2. Smith+Nephew 2019. Verification testing of Usability related design inputs for PRIMAFIX/CUTIFIX & PRIMAFIX Tender. Internal report. U/073/R2. 3. Smith+Nephew 2011. PRIMAFIX Product Claims Transfer Report. Internal report. CCA1936/R1. 4. Smith+Nephew 2020. Determining the radio-transparency of PRIMAFIX dressings using a Surgical C-Arm X-ray imaging machine. Internal report. WRQ-PCS100-377.