

Quick set-up guide




Remove handset from carton



Open external pouch



Prepare internal pouch for transfer

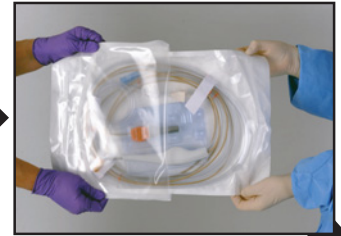


Transfer inner pouch to sterile field



Remove device contents



Prepare device. Transfer saline tube, evacuation tube and pump from sterile field

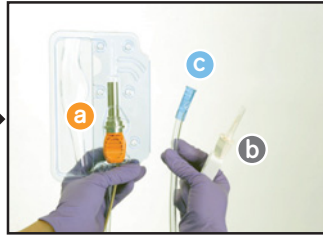

a. Handset pump cartridge
 b. Saline spike line
 c. Evacuation line



Remove pump cartridge from clam shell



Turn console power ON




Insert pump cartridge into console




Turn right to 3 o'clock



Remove saline tube spike cap

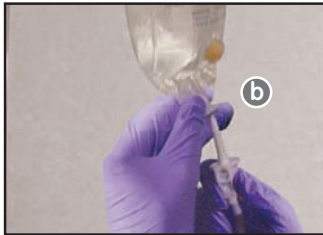


Spike saline (3L) bag. Ensure saline reaches handset before engaging foot pedal

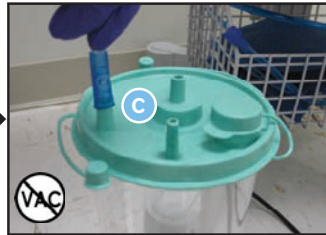

Attach evacuation tube to vented canister



Increase power setting to 10 for priming

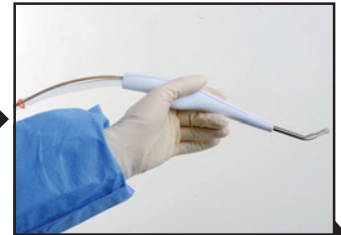

Safely hold handset



Depress foot pedal to prime



Reduce power to desired procedure setting



Ready

Pump cartridge difficult to remove



First option, turn console off. Try to remove



Second option, turn to unlocked position and gently push cartridge into console a little further. Quickly remove hand allowing cartridge to spring back before trying to remove



Third option, clamp saline line and remove spike from bag. Hold line and adjust power setting to 10, then open the line. Press foot pedal until water jet stops streaming in operating window. Try to remove

Failure conditions



Press and hold up/down keys simultaneously. F1 means power supply failure has occurred. Replace console



F2 means an internal motor failure has occurred. Replace console



F3 means an over-heated failure has occurred. Allow console to cool 10 minutes leaving bottom and back ventilation clear

To replace console, email endoreturn@smith-nephew.com and customer care.largo@smith-nephew.com the following items:
1) Completed VERSAJET II complaint form
2) No charge PO#
3) Console serial number


A return authorization number (RA#) and a decontamination form will be sent to you. Upon receiving your replacement or loaner console, please use its shipper box to return the inoperable console. Please attach the completed decontamination form onto the shipper box and send to:

Smith & Nephew
76 S. Meridian Ave.
Dock #1/Complaint
Oklahoma City, OK 73107

Handset doesn't prime




Verify pinch clamps are fully open

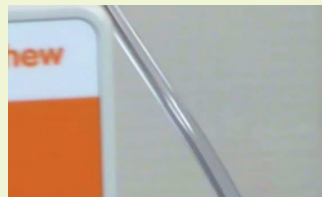

Check for kinks, obstructions or leaks in the inflow line



Set power level to 10. Press foot switch and pinch the clamp. Drag it down to purge all air from the feed line

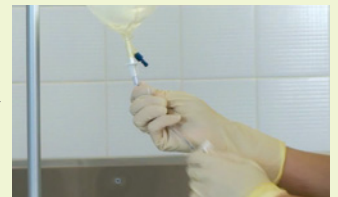

User tips



Keep handset moving tangentially at swift and steady pace to prevent grooves in the woundbed



Invert handset away from wound when procedure is finished, then remove foot from footswitch to prevent residual saline from trickling back into the clean wound bed

